


PROPERTY OF NS.
PLEASE RETURN


297-3601



1017

MODEL 800
STANDARD SIGNAL GENERATOR

Operating
INSTRUCTIONS

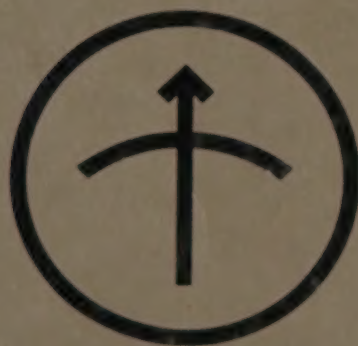

MP MASTER



MA25130

MEASUREMENTS

A MCGRAW-EDISON DIVISION

BOONTON

NEW JERSEY

MEASUREMENTS

BOONTON

NEW JERSEY



MODEL 800
SERIAL # 264
11 NOV 69

SUPPLEMENTARY SHEET

MEASUREMENTS 801
STANDARD SIGNAL GENERATOR

The Model 801 Standard Signal Generator is equivalent to the Model 800 described by this instruction manual, except a new frequency range, 68 to 88 MHz, has been added and the frequency range 890 to 960 MHz has been deleted.



Digitized by the Internet Archive
in 2025

https://archive.org/details/manualsplus_06210

**MODEL 800
STANDARD SIGNAL GENERATOR**

Operating
INSTRUCTIONS

NO PART OF THIS MANUAL MAY BE
REPRODUCED IN WHOLE OR IN PART
EXCEPT BY PERMISSION OF
MEASUREMENTS

COPYRIGHT 1969 BY MEASUREMENTS
Printed in U.S.A.

MEASUREMENTS

A MCGRAW-EDISON DIVISION

BOONTON

NEW JERSEY

TABLE OF CONTENTS

	PAGE
Foreword	1
Front View of Model 800	2
Section I INTRODUCTION	3
A. Scope of Manual	3
Section II DESCRIPTION AND DATA	3
A. General	3
B. Technical Characteristics	3
C. Design Features	7
D. Components Supplied	9
E. Packaging	9
Section III CONTROL FUNCTIONS	10
A. Power	10
B. Tuning Dial	10
C. Ext. Mod.	10
D. Output Control	11
E. Mod. Switch	11
F. Dev. Control	12
G. Meter	12
Section IV SERVICE UPON RECEIPT OF INSTRUMENT	13
A. Preliminary Inspection	13
Section V OPERATION	14
A. Operating Procedure	14

	PAGE
Section VI	MAINTENANCE
	16
A.	General Precautions
	16
B.	Removal of Instrument From Case
	17
C.	Removal of Front Panel
	17
D.	Lamp Replacement
	18
E.	Power Supply Adjustments
	18
F.	R.F. Osc. Tube Replacement
	19
G.	R.F. Osc. Voltage Variable Capacitor Replacement
	21
H.	R.F. Osc. Bolometer Replacement
	22
I.	Automatic Output Board Adjustment
	24
J.	Output (Incr. Dist. Board Pt. 3) Adjustment
	25
K.	Deviation Amplif. Board Adjustment
	26
L.	Deviation Adj. Board Adjustment
	27
M.	Distortion (Incr. Dist. Board Pt. 2) Adjustment
	28
N.	Incremental (Incr. Dist. Board Pt. 1) Adjustment
	29
O.	Audio Osc. Board Adjustment
	30
P.	Saw-tooth Board Test
	31
Section VII	EQUIPMENT USED WITH MODEL 800
	32
A.	Accessories and Auxiliary Equipment
	32
Section VIII	STORAGE AND SHIPMENT
	33
A.	Storage
	33
B.	Shipment
	33
Section IX	REPLACEABLE PARTS
	34

Section X PRINTED CIRCUIT BOARD PARTS LAYOUT

A. Power Supply Board	47
B. Audio Osc. Board	48
C. Incr. Dist. Board	49
D. Saw-tooth Board	50
E. Deviation Amplif. Board	51
F. Deviation Adj. Board	52
G. Automatic Output Board	53

APPENDIX I SCHEMATIC DIAGRAM

APPENDIX II CALIBRATION CHART

FOREWORD

Additional information with regard to the applications and maintenance of this equipment will be available from time to time. Users of the Model 800 Standard Signal Generator are urged to discuss their problems with us and to suggest such modifications as might make the instrument more adaptable to their special requirements.

Whenever possible, maintenance difficulties should be reported to MEASUREMENTS before proceeding with the actual repairs. Through our familiarity with the instrument, we are in a position to suggest the most expedient and accurate repair procedure.

Your Model 800 Standard Signal Generator has been designed and manufactured to the highest standards of instrument quality. With reasonable care, many years of trouble-free service can be expected of it.

Engineering Department

MEASUREMENTS

A Mc-Graw Edison Division

Box 180

Boonton, New Jersey 07005



Figure 1. Front View of the Model 800 Standard Signal Generator

SECTION I

INTRODUCTION

A. SCOPE OF MANUAL

a. This manual describes the basic operation and maintenance of the Model 800 Standard Signal Generator. Also included are the recommended procedures for preparing the instrument for reshipment or for prolonged storage, and a list of replaceable parts.

SECTION II

DESCRIPTION AND DATA

A. GENERAL

a. The Model 800 Standard Signal Generator is a portable test equipment for checking the operation of mobile communication receivers. CW or frequency-modulated carrier may be selected as required.

B. TECHNICAL CHARACTERISTICS

a. Carrier frequency ranges.

(1)	<u>Frequency</u>	<u>Band Letter</u>
	25 - 32 MHz	A
	32 - 41 MHz	B
	41 - 54 MHz	C
	130 -175 MHz	D
	400 -470 MHz	E
	890 -960 MHz *	F

- * Band F dial is calibrated on the second harmonic of the 445 to 480 MHz range.

(2) The Range Switch operates a mask to expose the frequency in use.

b. Frequency Accuracy.

(1) Each range is individually calibrated to an accuracy of $\pm 0.5\%$.

c. Tuning.

(1) A Coarse Tuning Knob is geared to the main frequency dial. This knob may be set to place its indicator at zero at any desired frequency.

(2) A Fine Tuning Knob electronically fine tunes the oscillator.

d. Output Voltage

(1) The output voltage is continuously variable from 100,000 microvolts to 0.1 microvolt. The output is also calibrated from -8 to -128 DBM. (0 DBM is one milliwatt into 50 ohms). An individually calibrated correction curve is supplied for band F.

(2) A pad mark is provided on the fiducial so that the output may be read directly when a 2 to 1 voltage-ratio (6 db) pad is employed.

(3) The output is calibrated in terms of the voltage developed across a 50-ohm resistive termination.

e. Output System

(1) The mutual inductance attenuator is of the wave-guide-below-cut-off type. This attenuator has excellent incremental calibration accuracy determined by its physical dimensions which are held to close tolerances.

(2) The output voltage reference level is continuously monitored by a temperature-compensated barretter bridge.

(3) The output of the barretter bridge controls the automatic output level adjusting circuit. The 100,000 microvolt reference level is accurate to $\pm 10\%$ from 25 MHz to 470 MHz; an output chart is provided for 890 to 960 MHz.

(4) To improve reliability, no resistor is used in series with the output pick-up loop. Inadvertently operating the press-to-talk button when servicing Mobile equipment could burn out such a resistor. An external pad, Measurement's Part No. 80-ZH1 or 80-ZH3, may be used to improve the VSWR of the output system.

f. Shielding.

(1) Double shielding is used on the oscillator to reduce stray radiation to a low value.

(2) Multi-section individually-shielded r.f. filters are used on all circuits supplying the oscillator.

(3) Carrier leakage is negligible on all frequency ranges.

g. Modulation.

(1) The Model 800 is an FM signal generator utilizing variable-capacitance diodes in the frequency modulator.

(2) An internal 1000 hertz Wien bridge RC oscillator provides modulation voltage. Peak deviation may be varied from zero to 16 kHz.

The Model 800 may also be externally modulated. approximately 1V rms is required for 16 kHz deviation. Frequency deviation response is within 1 db from d.c. to 15 kHz.

(3) An internal 20 Hz saw-tooth generator provides continuously adjustable metered sweep width up to 32 kHz peak-to-peak.

(4) Internal DC modulation voltages provide metered INCREMENTAL Carrier shifts up to 16 kHz each side of carrier.

h. Residual Modulation.

(1) Residual FM modulation is less than 100 hertz at 460 MHz.

(2) Regulated d-c power supplies are used for the plate and the heater of the oscillator tube.

1. Deviation.

(1) Peak deviation is indicated directly on the panel meter for all bands.

(2) Deviation accuracy is within $\pm 10\%$ of full scale.

(3) Means are provided for manually shifting the carrier frequency ± 16 kilohertz (INCREMENTAL) to facilitate discriminator alignment. This is accomplished by varying the d-c potential applied to the variable-capacitance diodes. The frequency shift, in kilohertz, is indicated by the panel meter.

j. Power Supply Source.

(1) Potential 115 or 230 volts $\pm 10\%$.

(2) Frequency 50 or 60 cycles.

(3) Power Consumption 16 watts.

C. DESIGN FEATURES

a. The electrical and mechanical design of the Model 800 Standard Signal Generator is based upon many years of experience gained in manufacturing thousands of Standard Signal Generators. The Model 800 is a standard of radio frequency voltage. It generates an accurately calibrated voltage at an accurately calibrated frequency. Solid state circuitry is used wherever practical to reduce operating temperature and improve stability.

b. In accordance with Measurement's policy of maintaining high-quality features in instruments, the Model 800 uses a temperature-compensated barretter bridge for continuously monitoring and controlling the level of the output voltage. The barretter bridge is the most accurate standard presently available for RF voltage measurement and, because of its response, insures a high degree of absolute voltage accuracy. It is superior to a crystal diode in its stability, its freedom from errors due to temperature changes, and in its excellent long-term stability.

c. RF leakage is negligible and microphonics have been minimized to make the Model 800 suitable for checking the most sensitive receiver.

d. A solid state internal oscillator provides a 1000 Hz modulation frequency. Modulation from an external source may also be used.

e. A solid state internal 20 Hz saw-tooth generator provides linear carrier sweep up to 32 kHz peak-to-peak as indicated on the internal modulation meter.

f. The type 6DV4 oscillator nuvistor is readily available. Its use in the Model 800 is attractive from the service viewpoint.

g. Regulated and well filtered direct-current power supplies are used for oscillator plate and heater to provide good frequency stability and to minimize residual FM due to power frequency hum. The power transformer is floated on rubber mounts to reduce power-line-frequency mechanical vibration of the oscillator components.

h. The frequency bands have been designed to give excellent band spread by using a tuning ratio of approximately 1.3 to 1. This small tuning range permits the use of a variable capacitor with heavy rotor plates and wide plate spacing to reduce microphonics to a minimum.

i. Frequency modulation is produced by two variable-capacitance diodes connected across the stator plates of the tuning capacitor through adjustable trimmer capacitors to obtain optimum Q, low distortion, and maximum stability.

j. Deviation compensation is provided by a tracking potentiometer ganged to the tuning dial and individual level-setting potentiometers for each frequency band. The deviation is indicated directly on the panel meter for all bands.

k. A means is provided for incremental change in carrier frequency to facilitate discriminator alignment. This is accomplished by varying the d-c potential applied to the variable-capacitance diodes. The frequency shift, in kilohertz, is indicated by the panel meter.

l. Electronic Fine Tuning is provided enabling very fine adjustment of carrier frequency with or without modulation.

D. COMPONENTS SUPPLIED

a. The following is included with each shipment:

1 Model 800 Standard Signal Generator

Approx. Weight	24# with transit cover
Height	14 1/2"
Width	10 1/2"
Depth	9 1/2"
Volume	1.1 cu. ft.

1 Manual of Operating and Maintenance Instructions

1 Tube, Nuvistor 6DV4 installed.

1 Tube, Regulator 5651A installed.

E. PACKAGING

	<u>Domestic</u>	<u>Export</u>
Approx. Weight	34#	62#
Height	15"	17"
Width	20 1/2"	22"
Depth	12 1/2"	17"
Volume	2.3 cu. ft.	3.7 cu. ft.

For export shipment the Model 800 is packed in a wooden shipping container.

SECTION III

CONTROL FUNCTIONS

A. POWER

a. The ON-OFF Switch controls the application of line voltage to the primary of the power transformer.

b. The FUSE (located at the rear of the instrument) protects against overloads.

B. TUNING DIAL

a. The RANGE Knob selects one of the six frequency ranges. The range letter and frequency appears in the window above the knob as it is rotated.

b. The COARSE TUNING Knob sets the desired carrier frequency. The frequency is directly indicated under the fiducial line in the panel opening directly above the RANGE Knob. The Frequency Dial will automatically disengage when the usable part of the tuning range has been passed. To facilitate selectivity measurements about any center frequency the Frequency Dial may be disengaged from the tuning mechanism by pressing the Coarse Tuning Knob to the right. The Coarse Tuning Knob may then be rotated so that it may be placed at zero with reference to its calibration marks.

c. The FINE TUNING Knob electronically fine tunes the carrier.

C. EXT. MOD.

a. The EXT. MOD. binding posts on the left side of the panel permit the application of an external signal for frequency modulation of the carrier.

b. Approximately 16 kHz FM deviation is produced per 1.0V rms of modulating signal. The deviation is indicated on the panel meter.

D. OUTPUT CONTROL

a. The OUTPUT Control is a dial calibrated in MICROVOLTS and DBM. This dial adjusts the position of the output loop in the piston attenuator and will indicate the true output in MICROVOLTS or DBM when the R.F. OUTPUT connector is terminated in a 50 ohm resistive load.

b. In order to check the output R.F. level, the MOD. switch must be in the CW position. This connects the meter to the output bridge circuit. When the MOD. switch is in any other position, the meter is disconnected from the barretter bridge and is used to indicate frequency deviation.

c. When a 50 ohm, 6 db pad is connected between output connector and 50 ohm load resistor, the output level is read directly beneath the pad line on the plastic fiducial.

E. MOD - DEV SWITCH

a. The MOD - DEV Switch is located directly below the meter. Its purpose is to supply the carrier signal with the type of modulation desired.

(1) The EXT. position allows external modulation to be applied to the oscillator via the two EXT. MOD. binding posts located at the left side of the front panel. The deviation is indicated on the panel meter.

(2) The CW position provides an unmodulated continuous-wave carrier. In this position the panel meter is connected to the balometer bridge for R.F. voltage level checking.

(3) The 1000 hertz position applies approximately 1V rms to the modulator input for internal 1000 Hz modulation.

(4) The INCR. position permits incremental adjustment of the carrier frequency.

(5) The SAW-TOOTH position applies a sweep voltage to the modulator input for internal modulation. The saw-tooth wave-form is also available from the EXT. MOD. binding posts for application to the horizontal or sync. input of an oscilloscope.

F. DEV. CONTROL

a. The DEV. Control is a potentiometer which controls frequency deviation when either internal or external modulation is employed. It also adjusts incremental frequency shift. It is operated by the smaller knob on the MOD - DEV switch.

b. The frequency deviation, or incremental frequency shift, is indicated on the panel meter.

G. METER

a. The meter is used to check the reference level of output voltage and also to measure deviation.

b. When the MOD - DEV switch is in the CW position, the meter is connected to the barretter bridge to monitor the R.F. output level.

c. When the MOD - DEV switch is in any other position, the meter is disconnected from the barretter bridge and indicates frequency deviation in kHz. In this case the meter is connected to a crystal diode rectifier and operates as an a-c voltmeter.

d. When the MOD - DEV switch is in the INCR. position, the meter indicates incremental shift in carrier frequency.

SECTION IV

SERVICE UPON RECEIPT OF INSTRUMENT

A. PRELIMINARY INSPECTION

a. The following preliminary checks will indicate whether or not the instrument is operating properly.

(1) Connect the power cord to a power source of 115 volts 50-60hertz alternating current (unless a special nameplate is attached to the instrument indicating that it has been wired for 230 volts 50-60 hertz operation). Turn the power ON and note whether the Frequency Dial and Meter are illuminated. If not, check the line cord connections and fuse. If the fuse is defective replace it with a new Type MDL slow blow fuse.

(2) Allow about ten minutes for the instrument to stabilize.

(3) Rotate the RANGE Knob until the letter "A" appears in the window above the knob. Rock the knob slightly from side to side to make certain that the range change mechanism has locked into position.

(4) Place the MOD - DEV Switch in the CW position. The meter pointer should rest on the LEVEL BALANCE mark on the meter dial.

(5) Repeat steps a.3 and a.4 for each frequency range.

(6) Place the MOD - DEV Switch in the 1000 position and rotation the DEV control from full counterclockwise to the full clockwise position. The Meter pointer should deflect from zero to full scale.

SECTION V

OPERATION

A. OPERATING PROCEDURE

a. Connect the power cord to a source of 115 volt 50-60 hertz alternating current (unless a special nameplate is attached to the instrument indicating that it has been wired for 230 volt 50-60 hertz operation). Place the ON-OFF Switch in the ON position. Allow about ten minutes for the instrument to become stabilized.

b. Rotate the RANGE Knob to select the desired frequency band.

c. Set the COARSE TUNING knob to the desired carrier frequency and adjust the FINE TUNING knob as necessary for critical frequency adjustment.

d. Turn the MICROVOLTS dial to the desired output voltage as indicated under the fiducial line.

e. To frequency modulate the carrier, set the MOD - DEV Switch to EXT. 1000 INCH., or Saw-tooth as desired. Rotate the DEV. control to desired kHz DEVIATION as indicated on the meter.

f. To frequency modulate the carrier using external modulation, connect the modulating signal to the EXT. MOD. binding posts. This signal should be approximately 1V rms to produce the full 16 kHz of deviation. Set the MOD - DEV Switch to EXT. and rotate DEV. control to desired kHz DEVIATION as indicated on the meter.

g. If incremental control of carrier frequency is desired, set MOD - DEV Switch to INCR. The DEV. control adjusts the frequency shift, as indicated on lower scale of the meter.

h. For all frequency bands, the deviation in kHz is indicated on the panel meter to an accuracy of $\pm 10\%$ of full scale.

SECTION VI

MAINTENANCE

A. GENERAL PRECAUTIONS

a. The purpose of this section is to acquaint operating and maintenance personnel with procedures for making certain adjustments that may be necessary after tube or critical parts are replaced.

b. It should be noted that most of the field replaceable parts are available from Measurements. Please refer to Measurements part numbers when ordering. Pre-tested and preadjusted plug-in printed circuit boards are also available. These generally require very slight readjustment after installation. The adjustment procedures outlined in this section should be carefully followed. When the described test equipment is not available, it would be advisable to return the Model 800 to Measurements for repair.

c. The following precautionary procedures should be observed if the Model 800 is opened for examination:

(1) Do not attempt to readjust any controls not specifically described in the following paragraphs.

(2) Do not use an ohmmeter or other source of current without first unsoldering one terminal of each of the Bolometer Assemblies. These Bolometer elements are easily burned out and difficult to replace.

(3) The instrument should not be grounded during a soldering operation because of possible electrical leakage in soldering irons.

(4) Exposed portions of the calibrated Carrier Frequency Dial should be protected against handling. No liquids should be

used for cleaning this dial.

B. REMOVING THE INSTRUMENT FROM THE CASE

a. Disconnect the power cord from the AC source.

b. Turn the MICROVOLTS Dial clockwise to the 100,000 microvolts position.

c. With the instrument in its normal upright position, remove six Phillips head screws nearest the front edge of the case. Two on each side, one on the top and one on the bottom. Break sealing wax on the bottom screw. The front section of the instrument is now free of the case except for the cable connecting it to the power supply chassis.

d. Gently tip the top of the instrument forward so that the edges of the front panel may be grasped with the hands. Remove instrument from the case.

e. Lay the instrument face down supporting the edges of the panel on a pair of 2" X 4" wood blocks or equivalent. Allow clearance so that no weight rests on the control knobs.

f. The Power Supply Assembly may be removed from the case by removing the six Phillips head screws holding it into the case.

C. REMOVING THE FRONT PANEL

a. Place the instrument with the top edge of the panel down.

b. Remove the Range, Coarse and Fine Tuning and Mod-Dev knobs.

c. Remove the clear plastic fiducial which is located above the Microvolts Dial. Remove the Microvolts Dial.

- d. Remove the connections from EXT. MOD. posts.
- e. Disconnect the leads from the Meter. Mark the leads so that they may be properly replaced.
- f. Remove the six Phillips head 6-32 screws (2 nickel and 4 black) from face of panel. The front panel is now free of the front section.

D. LAMP REPLACEMENT

If lamp replacement is indicated, proceed as follows:

(1) For Meter Lamp replacement remove the instrument from the case. Remove bayonet 6 volt lamp and replace with a GE #44 lamp or equal.

(2) For Carrier Frequency Dial Lamp replacement remove the instrument from the case and remove the front panel. Remove the bayonet 6 volt lamp and replace with a GE #44 lamp or equal.

E. POWER SUPPLY ADJUSTMENT

a. Remove the instrument and power supply from the case, exposing the numbered pin connections on the underside of the power supply connector mounted on the power supply chassis. With the instrument connected to the power supply and with the power supply connected to an adjustable source of A.C. power:

(1) Adjust A.C. line voltage to 115 VAC (Note: Some instruments are prewired to operate on 230 VAC - adjust accordingly).

(2) Switch instrument power switch "ON".

(3) Using an accurate ($\pm 3\%$ or better) high impedance V.O.M. (20,000 ohms per volt suggested) measure and adjust the three power supply voltages as indicated. Do not readjust power supply voltages if within $\pm 3\%$ of nominal values. A slight change in adjustment could effect the adjustment of other circuits:

<u>Voltage</u>	<u>Test Point On Connector</u>	<u>Adjustment Control</u>
(adjust 1st) + 115V DC	pt 3 to ground 4	+ 115V ADJ.
(adjust 2nd) + 12V DC	pt 2 to ground 4	+ 12V ADJ.
(adjust last) - 6.3V DC	pt 1 to ground 4	- 6.3V ADJ.

(4) Vary line voltage ± 15 VAC. The + 115V DC and + 12V DC supplies will not vary noticeably over this range. The - 6.3 VDC supply will vary up to 0.1 VDC.

(5) If a high sensitivity oscilloscope or VTVM is available, check residual hum and noise of the three power supplies:

- + 115V DC - less than 5 mv rms.
- + 12V DC - less than 1 mv rms.
- 6V DC - less than 1 mv rms.

NOTE

ADJUSTMENT OF THE POWER SUPPLIES AFFECTS MANY OTHER ADJUSTMENTS THROUGHOUT THE MODEL 800. IT IS IMPORTANT THEREFORE, THAT THE REMAINDER OF THE MEASUREMENTS DESCRIBED IN THIS SECTION BE PERFORMED AND ADJUSTMENTS MADE AS INDICATED.

F. R.F. OSCILLATOR TUBE REPLACEMENT

- a. If replacement of the Oscillator Newistor Tube #101

is indicated, proceed as follows:

(1) Remove the strap holding the oscillator shield covers.

(2) Twist off the outer and inner shield covers. Tools must never be used to pry off these covers as even slight dents in the cans or covers may cause serious leakage of the carrier.

(3) Remove the lower screw from roller spring on top of the coil disc and retract the upper screw sufficiently to permit roller to be removed. Rotate the spring to clear the coil disc.

(4) Rotate coil disc to place detent roller midway between detent positions.

(5) Hold coil disc firmly and remove nut which secures the coil disc (use a 1" spanner wrench).

(6) Lift the detent roller clear of disc edge and carefully lift coil disc assembly from its hub. The oscillator tube is now available for replacement. If possible, select a tube which has the least effect on the frequency calibration.

(7) Retract the detent roller, making certain its spring is engaged. Lower the coil disc in proper position to engage the flatted portion of the coil disc nut. Release detent roller against the edge of coil disc and rock disc until it is properly seated. Replace the coil disc nut and tighten firmly.

(8) Replace the roller, insert the lower roller spring screw and tighten both screws.

(9) Check alignment of the three coil contacts with their respective contact posts on the capacitor assembly since misalignment may cause serious damage.

(10) Replace the oscillator shield cans making certain that the factory marks line up on each cover and shield. Replace the holding strap.

G. R.F. OSCILLATOR VOLTAGE VARIABLE CAPACITOR REPLACEMENT

CAUTION

The voltage variable capacitors used in the Model 800 have seldom been a cause of trouble. Throughout the years Measurements has produced many thousands of Signal Generators employing similar or identical modulators. Although the voltage variable capacitors have often been suspected of causing noise, instability and even hum in the Signal Generators, the problems could almost invariably be traced to other causes. Installation and adjustment of the voltage variable capacitors is particularly critical and should only be performed after very careful consideration.

a. Remove the R.F. Oscillator shield covers and coil disc as described in Par. F.

b. Unsolder and replace the entire Voltage Variable Capacitors assembly including C102 and C105 trimmer capacitors, Voltage Variable Capacitors C103 and C104, and 150 K resistors R103, R104, and R105. The trimmer closest to the panel (C102) should be preset to 1 pf., before the assembly is installed in the oscillator.

- c. Replace the coil disc assembly as described in Par. F.
- d. Set Generator to "A" Range and set frequency to 25 MHz.
- e. Modulate the oscillator using the internal 1000 Hz modulation (set to 16 kHz deviation).
- f. Using an external Standard Deviation Meter such as Measurements Model 140A or Model 920, measure the actual deviation.
- g. Adjust trimmer C105 until the actual deviation measures 16 kHz.

NOTE

The voltage at the wiper of section 3 of the Deviation Band switch should measure 6 VAC rms with approximately 55V DC bias and 16 kHz deviation. If not, set the deviation control to provide these voltages regardless of the internal modulation meter reading. Reset trimmer C105 to obtain 16 kHz deviation as measured on the external Deviation Meter. This will necessitate readjustment of the Deviation Adjust Potentiometers as outlined in Paragraph L of this section.

H. R.F. OSCILLATOR BOLOMETER REPLACEMENT

CAUTION

In testing the bolometer circuit, do not use an ohmmeter or other source of current without first unsoldering one terminal of each of the bolometer assemblies. The Bolometer elements are easily burned out and difficult to replace.

The instrument should not be grounded during a soldering operation because of possible electrical leakage in the soldering iron.

a. Remove R.F. Oscillator shield covers and coil disc as in Par. F., exposing the Bolometer block assembly.

b. Make careful note of the leaddress of the wires and cable leading to and from the bolometer block (including the wire passing through the sub-panel of the instrument).

c. Disconnect the resistance wire insulated leads from the filter terminals by unsoldering carefully.

d. Disconnect the wire which passes through the sub-panel to the r.f. choke by unsoldering the choke end.

e. Remove the three 6-32 screws which attach the block to the shields and sub-panel.

f. Gently remove the bolometer block, drawing the attached wire through the sub-panel. Allow the shielded cable to remain attached to the block.

g. Unsolder the lead attached to the bolometer through the leadwasher hole in the bottom of the block. Also detach the connection to the terminating resistor R109 through the access hole in the bottom of the block.

h. Loosen the 4-40 Allen head set screws and slide the bolometer assemblies from the block.

i. Reinstall repaired bolometer block assemblies into the block; resolder connections and retighten set screws. Be sure the lead washer slightly overlaps to insure positive seal of the shield and sub-panel hole.

j. Reinstall the bolometer block. Tighten the three mounting screws evenly to assure tight lead washer seal.

k. Reconnect all leads carefully and redress to minimize effects of leakage and spurious resonance.

l. Reinstall the Coil disc and the shield covers as described in Par. F.

I. AUTOMATIC OUTPUT BOARD ADJUSTMENT

a. Connect the R.F. output of the Model 800 through a Measurements Type H-5710 cable and Type 80 ZH3 (6 db) pad to the input of a Measurements Model 202C Standard Barreter Bridge.

b. Carefully adjust the mechanical zero of the Model 800 meter.

c. Disconnect the +115V DC lead from the R.F. filter capacitor C109. Insulate the lead from the grounded chassis.

d. Connect the output of an external variable power supply to C109. The power supply should be capable of supplying up to 25 ma. dc.

e. Turn the Model 800 Power ON to provide filament voltage to the oscillator nuvistor tube V101.

f. Set the output of the Model 800 to 0.1 volt on the attenuator dial.

g. Adjust the external power supply to provide a 50 mV reading on the Barreter Bridge.

h. With the Model 800 MOD Switch in the E.W. position; adjust the OUTPUT ADJ. pot on the INLR, DIST. printed circuit board until the Model 800 Meter reads zero.

1. Short the input to the bases of Q701 (on the AUTOMATIC OUTPUT printed circuit board) together. Be extremely careful to not short either of these points to ground or to any other point on the socket. This could instantly destroy the bolometers in the R.F. Oscillator circuit. Adjust the BAL. control R708 for zero reading on the Model 800 Meter.

j. Adjust BIAS control, R704, for a reading of 75V DC as measured at the output of Q703 using as accurate high impedance V.O.M. This voltage reading is available from the lead previously disconnected from C109.

k. Turn the Model 800 Power OFF and remove the external power supply.

1. Disconnect the short at the input to Q701.

m. Reconnect the output lead to C109.

n. Turn the power on and test each Range of the Model 800 to see that the meter "zeros" in the C.W. position. The output voltage measured at C109 should vary within the range of 75V DC to 105V DC in the normal control of output level.

o. If the readings on the Model 202C do not spread properly about the 50 MV reading, readjust the OUTPUT ADJ. accordingly. Retest the output throughout each frequency range.

J. OUTPUT (INCR. DIST. BOARD PT.3) ADJUSTMENT

a. Check each frequency range of the Model 800 with the MOD switch in C.W. to see that the Automatic Output Board and the R.F. Oscillator are functioning properly.

b. Connect the output of the Model 800 through a Measurements Type H-5710 cable and Type 50 ZH3 (6 db) pad to the input of a Measurements Model 202C Standard Barreter Bridge.

c. Set the Output Attenuator of the Model 800 to 0.1 volts (100 K uv). The reading on the temperature stabilized and "zeroed" Barreter Bridge should be 50 mv $\pm 10\%$.

d. Check each frequency range of the Model 800 for output voltage accuracy.

e. Adjust the OUTPUT ADJ., R309 located on the INCR. DIST. printed circuit board for optimum compromise of output accuracy over the frequency ranges of the Model 800. Allow a few seconds after each adjustment for the Automatic Output circuit to stabilize.

K. DEVIATION AMPLI. BOARD ADJUSTMENT

a. Attach a VTVM such as Measurements Model 162 or Model 162R to the collector of Q502 on the Dev. Ampli. Board. Set the meter to the +100V DC range.

b. Turn the Model 800 power on.

c. Turn the DEV. control on the Model 800 to maximum CCW in the EXT. modulation position.

d. Adj. BIAS II, R506, for a reading of 45V on the VTVM.

e. Turn the DEV. control of the Model 800 to mid-range and rotate control back and forth about a quarter of a turn. Adj. BIAS I, R507, for zero change in VTVM reading as the DEV control is rotated throughout its range.

f. If necessary readjust BIAS II, R506, for a 45V reading.

g. Repeat steps e and f until the conditions of reading.

45V with zero effect from DEV control rotation are met.

h. Switch MOD to the 1000 Hz position and increase the DEV control for a 16 kHz reading on the Model 800 meter.

i. The A.C. voltage at the base and collector of Q502 should be approximately 1V rms and 10V rms respectively.

L. DEVIATION BOARD ADJUSTMENT

a. Attach a VTVM such as Measurements Model 162 or Model 162R to the C124 filter capacitor on the shield can of the R.F. Oscillator.

b. Set frequency on 25 MHz to "A" RANGE and the Power switch ON.

c. Connect the Model 800 to a Measurements Model 140A or Model 920 Standard Deviation Meter.

d. Check to see that the actual deviation as measured with the Standard Deviation Meter matches the reading of the internal Model 800 at 16 kHz. If not readjust "A" band DEV. AD. R611. The voltage measured by the VTVM should be approximately 6V AC and 55V DC. If not, it probably will be necessary to readjust the R.F. Osc. Voltage Variable Capacitors as outlined in Par. G.

e. Measure deviation at 32 MHz on "A" Range and adjust R612.

f. Alternately measure and adjust R611 and R612 until the deviation accuracy is compromised over the entire "A" Range.

g. Accurately measure the DC voltage at C124 (25 MHz on "A" Range).

h. Adjust the DIST. ADJ., R307, located on the INCR. DIST. BOARD PT 2 until the voltage at the wiper of R307 exactly equals the voltage at C124.

i. Repeat step f, if necessary, to correct for the affect of the adjustment of the DIST. ADJ. R307.

j. Repeat steps g, h, and i until all conditions are satisfied. Note that the DIST. ADJ., R307, will not have to again be adjusted throughout the remainder of the procedure.

k. Set frequency to 32 MHz on "B" Range. Check deviation and adjust DEV. ADJ., R609, if necessary.

l. Alternately measure and adjust R607 and R610 until the deviation accuracy is compromised over the entire "B" Range.

m. Perform similar adjustments of Ranges "C", "D", and "E" with the associated DEV ADJS., until all are adjusted as in step l for "B" range.

n. Perform similar adjustment RANGE "F" but the actual deviation reading as measured by the Model 140A should be half of the indicated reading on the Model 800. This is due to the doubling effect in using the 2nd. Harm. as the calibrated output frequency of RANGE "F".

M. DISTORTION (INCR. DIST. BOARD PT2) ADJUSTMENT

a. The adjustment of the DIST.ADJ., R307 normally affects the accuracy of "A" RANGE deviation. Distortion Adjustment should not be attempted except as part of the Deviation Board Adjustment procedure. Refer to Par. L of this Section.

N. INCREMENTAL (INCR. DIST. BOARD PT 1.) ADJUSTMENT

- a. Attach a direct coupled oscilloscope through a high impedance probe from the wiper of the DEV. Control., R51, to ground.
- b. Establish a ground reference line at the vertical center of the oscilloscope.
- c. Switch the Model 800 Power ON and switch the MOD switch to the 1000 Hz position. Set the Dev. Control to 16 kHz.
- d. Adjust the vertical sensitivity of the oscilloscope so that, with the ground at center, the tips of the sinusoid are set to the highest and lowest graticule lines. Full scale on the oscilloscope will now correspond to the "peak-to-peak" deviation of 32 kHz (Note that the Model 800 is calibrated in terms of "peak" deviation).
- e. Switch the MOD switch to the INCR. position.
- f. Adjust INCR. CENT., R306, fully CCW.
- g. Rotate the DEV. Control to the point corresponding to ground on the oscilloscope. This should also cause a zero reading on the Model 800 Meter. (-16 kHz on the INCR. scale).
- h. Readjust the INCR. CENT., R306, for "0" INCR. reading on the Model 800 Meter.
- i. Adjust the INCR. ADJ., R304, so that full scale reading on the oscilloscope corresponds to full scale +16 kHz and -16 kHz on the Model 800 Meter when the DEV control is rotated.
- j. Repeat adjustment of the INCR. CENT., R306, and INCR. ADJ., R304 so the full scale readings on the oscilloscope correspond to full scale +16 kHz and -16 kHz on the Model 800

meter and also that the ground reading on the oscilloscope corresponds to zero on the meter. The two adjustments are interdependent and generally require back and forth adjusting a few times until all of the three conditions are satisfied.

O. AUDIO OSC. BOARD ADJUSTMENT

a. Connect the high impedance probe of an oscilloscope to the EXT binding posts of the Model 800.

b. Switch the Power ON and the MOD switch to the 1000 Hz position. Decrease the BIAS ADJ., R206, on the Audio Osc. Board until the oscillator drops out of oscillation. Increase the BIAS ADJ., R206 until slightly beyond where the oscillations start again. (Note that a few seconds are required for the oscillator to stabilize each time the oscillation starts).

c. Attach an audio counter to the EXT. binding posts and measure the frequency of oscillation. Adjust the FREQ. ADJ., R207 for exactly 1000 hertz on the counter.

d. Readjust the BIAS ADJ., R206, as in steps a & b and test the starting of the oscillator by switching the MOD switch in and out of the 1000 Hz position. If the oscillator is sluggish starting, advance the BIAS ADJ., R206, slightly.

e. Observe the waveshape of the 1000 Hz sinusoid on the oscilloscope. The waveshape should be undistorted and greater than 3.5V peak-to-peak.

f. Connect a harmonic distortion analyzer to the EXT binding posts. Harmonic distortion should measure less than 0.5%.

R. SAW-TOOTH BOARD TEST

- a. Attach a direct-coupled oscilloscope to the EXT. binding posts.
- b. Switch the Power ON and the MOD switch to the Saw-tooth position.
- c. Observe the waveform of the saw-tooth as viewed on the oscilloscope. The Model 800 Saw-tooth waveform should be linear providing that the oscilloscope sweep circuit is also suitably linear.
- d. Advance the DEV Control to maximum. The reading should be well beyond full scale on the Model 800 Meter. The amplitude of the Saw-tooth as measured on ~~the~~ oscilloscope should be greater than 3 volts peak-to-peak.

SECTION VII

EQUIPMENT USED WITH MODEL 800

A. ACCESSORIES AND AUXILIARY EQUIPMENT

a. Accessories.

(1) Type 80-ZH-1 Output Matching Pad, 6 db loss, with Type N Input Connector and UHF Output Connector.

(2) Type 80-ZH-3 Output Matching Pad, 6 db loss, with Type N Input Connector and Type N Output Connector.

(3) Type M-342 Output Matching Pad, 10 to 1 voltage ratio (20 db), 50 ohm to 50 ohm for use from DC to 1000 MHz. Type N Input Connector and Type N Output.

(4) Type H-6080 Cable consisting of 4 ft. of RG-55/U with Type UHF Connectors at both ends.

(5) Type H-5710 Cable consisting of 4 ft. of RG-55/U with Type N Connectors at both ends.

(6) Type 84-Z2-2 Cable consisting of 4 ft. of RG-1/U with Type N Connector at one end and UHF Connector at other end.

(7) Type 80-ZH-4 Cable consisting of 4 ft. of RG-55/U with Type N Connector at one end and a pair of 3/4" spaced binding posts terminated in 50 ohm resistor at other end.

b. Auxiliary Equipment.

(1) Model 202-C Standard Barretter Bridge.

(2) Model 111-B Crystal Calibrator.

(3) Model 140A Standard Deviation Meter or Model 920 Standard Deviation Meter.

(4) Model 162, or 162R Vacuum Tube Voltmeter.

SECTION VIII

STORAGE AND SHIPMENT

A. STORAGE

- a. Remove dust from controls and outer surface of instrument with a clean rag.
- b. Wrap instrument in heavy wrapping paper and seal seams with gummed tape or similar adhesive.
- c. Store in a dry place. If excessive humidity is unavoidable, the wrapped instrument should be placed in a moisture-proof bag with a sufficient quantity of drying agent, such as silica gel, to insure a dry atmosphere. When the use of bag and desiccant is necessary, the instrument should be checked at six-month intervals to determine the effectiveness of the seal.

B. SHIPMENT

- a. Wrap the instrument with heavy wrapping paper and seal seams with gummed tape or similar adhesive.
- b. Place in fibre-board carton or wooden box large enough to permit at least three inches of excelsior or similar packing material between the instrument and sides of the box. For export packing, the instrument must be wrapped in water-proof paper and the seams sealed with waterproof glue or similar sealing compound before being placed in a wooden box.

SECTION IX

TABLE OF REPLACEABLE PARTS

Model 800 Standard Signal Generator

Measurements					
<u>Symbol</u>	<u>Part Number</u>	<u>Description</u>			
<u>Capacitors</u>					
C1	H-6617	Elect.	20-20-20.	mf	
2	H-6671-11	Ceramic	100	mmf	5% NPO
3	H-7886-1	Mylar	.22	mf	
4	H-6619-6	Ceramic	5 K	mmf	GMV
5	H-7513-9	Elect.	10	mf	15V
6	H-7601-4	Elect.	1000	mf	15V
7	H-7601-4	"	1000	mf	15V
8	H-7601-4	"	1000	mf	15V
9	H-7513-9	"	10	mf	15V
10	H-7601-3	"	1000	mf	50V
11	H-7601-3	"	1000	mf	50V
51	H-7886-1	Mylar	.22	mf	
101	H-8025	Tuning Capacitor Assembly. Includes 11011 thru E.			
102	H-6643	Variable; Mica 0.8 to 10 mmf			
103	H-6600-3	Voltage-variable 12 mmf			
104	H-6600-3	"	"	12	mmf
105	H-6643	Variable; Mica 0.8 to 10 mmf			
106	H-6162	Fixed; Ceramic	10 K	"	
107	H-6162	"	"	10 K	"
108	H-6160	"	"	1 K	"

Model 800 Standard Signal Generator

<u>Symbol</u>	<u>Part Number</u>	<u>Description</u>				
<u>Capacitors</u>						
C100	H-5944	Fixed; Feed-thru;	1 K muf			GMV
110	H-5944	" "	1 K "			"
111	H-5944	" "	1 K "			"
112	H-5944	" "	1 K "			"
113	H-5944	" "	1 K "			"
114	H-5250	Fixed; Ceramic; disc	10 K muf			"
115	H-5944	Fixed; Feed-thru;	1 K muf			"
116	H-5250	Fixed; Ceramic; disc	10 K muf			"
117	H-5944	Fixed; Feed-thru	1 K muf			"
118	H-5944	" "	1 K "			"
119	H-5942	" "	100 "	20%		
120	H-5942	" "	100 "	20%		
121	H-6627	" Standoff	100 "	20%		
122	H-6627	" "	100 "	20%		
123	H-5942	Feed-thru	100 "	20%		
124	H-5942	" "	100 "	20%		
125	H-5944	" "	1 K "			GMV
126	H-5944	" "	1 K "			"
127	H-5562	" Standoff	1 K "			"
128	H-6629	" Ceramic	22 "	5%		NPO30
129	H-6629	" "	22 "	5%		NPO30
130	H-5944	" Feed-thru	1 K "			GMV

Model 800 Standard Signal Generator

<u>Symbol</u>	<u>Part Number</u>	<u>Measurements</u> <u>Description</u>			
<u>Capacitors</u>					
C201	H-8060-1	Fixed Film	.015 mf	10%	
202	H-8060-1	" "	.015 "	"	
203	H-7886-1	Mylar	.22 "		
204	H-7513-6	Elect.	10 "		25V
205	H-7886-1	Mylar	.22 "		
206	H-7886-1	"	.22 "		
401	H-7886-1	"	.22 "		
402	H-7513-8	Elect.	100 "		25V
501	H-7886-1	"	6 "		100V
502	H-7886-1	Mylar	.22 "		
701	H-7513-11	Elect.	100 "		25V

Model 800 Standard Signal Generator

<u>Symbol</u>	<u>Measurements Part Number</u>	<u>Description</u>
<u>Rectifiers</u>		
CR1		Rectifier MDA-920A-7
2		" MDA-920A-1
3		" MDA-920A-2
4		Diode 1N758A
CR301		Diode 1N270
<u>Lamps</u>		
E1	H-5582	Lamp 6V
2	H-5582	Lamp 6V
E201	H-5052	Lamp 120V 3W
<u>Fuse</u>		
F1	H-5018-16	Fuse 1/4 amp
<u>Connector</u>		
J1	HS-18-1&2	Binding Post & Cap.
2	HS-18-1&2	" " "
101		Part of W101
<u>Coils</u>		
L101		Part of Att. Assy. Not replaceable
102		" " " " " "
103	H-6168	Coil Assembly, Range A. 25-32 MHz
104	H-6170	" " " B. 32-41 "
105	H-6172	" " " C. 41-54 "
106	H-6175	" " " D. 130-175 "
107	H-5744	Coil; Choke; r.f. 50 uh 20%

Model 800 Standard Signal Generator

<u>Symbol</u>	<u>Measurements</u> <u>Part Number</u>	<u>Description</u>				
<u>Coils</u>						
L108	H-5744	Coil; Choke; r.f.	50 uh	20%		
109	H-1442	" " "	18 uh	"		
110	H-1442	" " "	"			
111	H-1442	" " "	"			
112	H-5538	" " "	15 uh	20%		
113	H-5538	" " "	"	"		
114	H-1441	" " "	14 uh	approx.		
115	H-6563	" Filter	400 uh	20%		
116	H-6563	" "	"	"		
117	H-6563	" "	"	"		
118	H-6563	" "	"	"		
119	H-1442	" Choke; r.f.	18 uh			
120	H-1442	" " "	"			
121	H-1442	" " "	"			
122	H-6109	" " "	150 uh	approx.		
123	H-5744	" " "	50 uh	20%		
	H-6538	Coil Assembly; Range E.	.400-470 MHz			
	H-6538	" " "	F. 890-960 MHz			

Meter

M1	H-7998	Meter	50 u amp
----	--------	-------	----------

Model 800 Standard Signal Generator

<u>Symbol</u>	<u>Measurements</u> <u>Part Number</u>	<u>Description</u>
---------------	---	--------------------

Transistors

Q	1	Transistor	2N4249
	2	"	2N4249
	3	"	2N4898
	4	"	2N5294
	5	"	2N3440
	6	"	2N3440
	7	"	2N4240
	201	"	2N4123
	202	"	2N4123
	203	"	2N4123
	401	"	2N2646
	402	"	2N5457
	501	"	2N3440
	502	"	2N3440
	503	"	2N3440
	701	"	TD 100
	702	"	TD 100
	703	"	2N4240
	704	"	2N3440

Model 800 Standard Signal Generator

<u>Symbol</u>	<u>Measurements Part Numbers</u>	<u>Description</u>					
<u>Resistors</u>							
R1	H-3728-101	Fixed Comp.,	100	ohms	10%	1/2W	
2	H-8062-050	Fixed W.W.	4	"		5W	
3	H03728-182	Fixed Comp.,	1.8 K	"	10%	1/2W	
4	H-3727-362	Fixed Comp.,	3.6 K	"	5%	1/2W	
5	H-8061-502	Var. Comp.,	5 K	"			
6	H-3727-912	Fixed Comp.,	9.1 K	"	5%	1/2W	
7	H-3731-103	" "	10 K	"	10%	1W	
8	H-3727-203	" "	20 K	"	5%	1/2W	
9	H-3727-204	" "	200 K	"	5%	1/2W	
10	H-3734-224	" "	220 K	"	10%	2W	
11	H-3728-223	" "	22 K	"	10%	1/2W	
12	H-3728-123	" "	12 K	"	10%	1/2W	
13	H-6692-B2002F	Fixed Film	20 K	"	1%	1/2W	
14	H-8061-502	Var. Comp.,	5 K	"			
15	H-6692-B6652F	Fixed Film	66.5 K	"	1%	1/2W	
16	H-3733-203	Fixed Comp.,	20 K	"	5%	2W	
17	H-8061-102	Var. Comp.,	1 K	"			
18	H-3728-101	Fixed Comp.,	100	"	10%	1/2W	
51	H-6634	Var. Comp.,	10 K	"			
52	H-3728-104	Fixed Comp.,	100 K	"	10%	1/2W	
53	H-8084-102	Var. Comp.,	1 K	"		2W	

Model 800 Standard Signal Generator

<u>Symbol</u>	<u>Measurements</u> <u>Part Number</u>	<u>Description</u>				
<u>Resistors</u>						
R101	H-5586	Var. W.W.	20 K ohms			
102	H-3728-473	Fixed Comp.,	47 K "	10%	1/2W	
103	H-3728-154	" "	150 K "	10%	1/2W	
104	H-3728-154	" "	150 K "	10%	1/2W	
105	H-3728-154	" "	150 K "	10%	1/2W	
106	H-3728-103	" "	10 K "	10%	1/2W	
107		Part of Cap. Assy.	C106			
108		" " "	" C107			
109	H-6685-23	Fixed; film	63 ohms	1%	1/2W	
110	H-3727-510	" Comp.,	51 "	10%	1/2W	
111	H-3731-102	" "	1 K "	10%	1W	
112	H-3731-222	" "	2.2K "	10%	1W	
113	H-3731-222	" "	2.2K "	10%	1W	
201	H-3728-103	" "	10 K "	10%	1/2W	
202	H-3728-154	" "	150 K "	10%	1/2W	
203	H-3728-103	" "	10 K "	10%	1/2W	
204	H-3727-562	" "	5.6K "	5%	1/2W	
205	H-3728-122	" "	1.2K "	10%	1/2W	
206	H-8061-501	Var. Comp.,	500 "			
207	H-8061-502	" "	5 K "			
208	H-3727-513	Fixed Comp.,	51 K "	5%	1/2W	
209	H-3728-103	" "	10 K "	10%	1/2W	

Model 800 Standard Signal Generator

<u>Symbol</u>	<u>Measurements</u> <u>Part Number</u>	<u>Description</u>					
<u>Resistors</u>							
R210	H-3728-103	Fixed Comp.,	10 K	ohms	10%	1/2W	
211	H-3728-102	" "	1 K	"	10%	1/2W	
212	H-3728-101	" "	100	"	10%	1/2W	
213	H-3727-201	" "	200	"	5%	1/2W	
301	H-3728-682	" "	6.8 K	"	10%	1/2W	
302	H-3727-162	" "	1.6 K	"	5%	1/2W	
303	H-3727-513	" "	51 K	"	5%	1/2W	
304	H-3728-253	" "	25 K	"	10%	1/2W	
305	H-3727-242	" "	2.4 K	"	5%	1/2W	
306	H-3728-102	" "	1 K	"	10%	1/2W	
307	H-8061-104	Var. Comp.,	100 K	"			
308	H-3727-242	Fixed Comp.,	2.4 K	"	5%	1/2W	
309	H-8061-101	Var. Comp.,	100	"			
401	H-3727-625	Fixed Comp.,	6.2 meg		5%	1/2W	
402	H-3727-202	" "	2 K	ohms	5%	1/2W	
403	H-3727-201	" "	100	"	5%	1/2W	
404	H-3727-201	" "	200	"	5%	1/2W	
405	H-3727-202	" "	2 K	"	5%	1/2W	

Model 800 Standard Signal Generator

<u>Symbol</u>	<u>Measurements</u> <u>Part Number</u>	<u>Description</u>				
<u>Resistors</u>						
R501	H-3727-303	Fixed Comp.,	30 K ohms	5%	1/2W	
502	H-3727-753	" "	75 K "	5%	1/2W	
503	H-3727-164	" "	160 K "	5%	1/2W	
504	H-3728-103	" "	10 K "	10%	1/2W	
505	H-3728-474	" "	470 K "	10%	1/2W	
506	H-3727-511	" "	510 "	5%	1/2W	
507	H-8061-103	Var. Comp.,	10 K "			
508	H-8061-251	" "	250 "			
509	H-3727-242	Fixed Comp.,	2.4 K "	5%	1/2W	
510	H-3728-103	" "	10 K "	10%	1/2W	
511	H-3727-304	" "	300 K "	5%	1/2W	
601	H-8061-103	Var. Comp.,	10 K "			
602	H-8061-103	" "	" "			
603	H-8061-103	" "	" "			
604	H-8061-103	" "	" "			
605	H-8061-103	" "	" "			
606	H-8061-103	" "	" "			
607	H-8061-103	" "	" "			
608	H-8061-103	" "	" "			
609	H-8061-103	" "	" "			
610	H-8061-103	" "	" "			
611	H-8061-103	" "	" "			
612	H-8061-103	" "	" "			

Model 800 Standard Signal Generator

<u>Symbol</u>	<u>Measurements</u> <u>Part Number</u>	<u>Description</u>				
<u>Resistors</u>						
R701	H-3727-431	Fixed Comp.,	430	ohms	5%	1/2W
702	H-3727-301	" "	300	"	5%	1/2W
703	H-3728-561	" "	560	"	10%	1/2W
704	H-8061-102	Var. Comp.,	1 K	"		
705	H-3728-154	Fixed Comp.,	150 K	"	10%	1/2W
706	H-3728-154	" "	150 K	"	10%	1/2W
707	H-3728-103	" "	10 K	"	10%	1/2W
708	H-8061-502	Var. Comp.,	5 K	"		
709	H-3728-103	Fixed Comp.	10 K	"	10%	1/2W
710	H-3727-203	" "	20 K	"	5%	1/2W
711	H-3727-203	" "	20 K	"	5%	1/2W
712	H-3727-203	" "	20 K	"	5%	1/2W
713	H-3727-203	" "	20 K	"	5%	1/2W
714	H-3728-102	" "	1 K	"	10%	1/2W
715	H-3728-103	" "	10 K	"	10%	1/2W
716	H-3731-333	" "	33 K	"	10%	1W
717	H-3731-333	" "	33 K	"	10%	1W
718	H-3731-103	" "	1 K	"	10%	1W
719	H-3727-203	" "	2 K	"	5%	1/2W

Model 800 Standard Signal Generator

<u>Symbol</u>	<u>Measurements Part Number</u>	<u>Description</u>
<u>Bolometer</u>		
RT101) 102)	H-710	Bolometer: Matched pair
<u>Plugs</u>		
P1	H-8085	Plug, Interconnecting Cable
2		Part of W1.
3		" " W1.
<u>Switch</u>		
S1	H-8073	Switch, power
2	H-7941	" Mod-Dev. Includes R51.
3	H-7940	" Band
<u>Transformer</u>		
T1	H-8011	Transformer
<u>Tubes</u>		
V1		Tube, electron Type 5651
V101		" " Type ^{6AV6} 6AV6
<u>Cables</u>		
W1	H-7746	Cord; power. Includes P2 & P3
W101	H-8055	Output Cable and Connector


Model 800 Standard Signal Generator

Measurements
Part Number


Description

(Printed Circuit Board Assemblies)

H-7945	Saw-Tooth Generator
H-7948	Deviation Amplifier
H-7951	Audio Oscillator
H-7954	Incr. Adj.
H-7960	Deviation Adj.
H-7963	Automatic Output
H-8020	Power Supply
H-7971	Output Dial & Knob Assy.
H-8086-4	Range Tuning Knob
H-8086-3	Coarse " "
H-8086-1	Fine " "
H-8086-2	Mod-Dev. Knobs. 2 Concentric Knobs
H 6685	Resistor k. t for 62b PAD

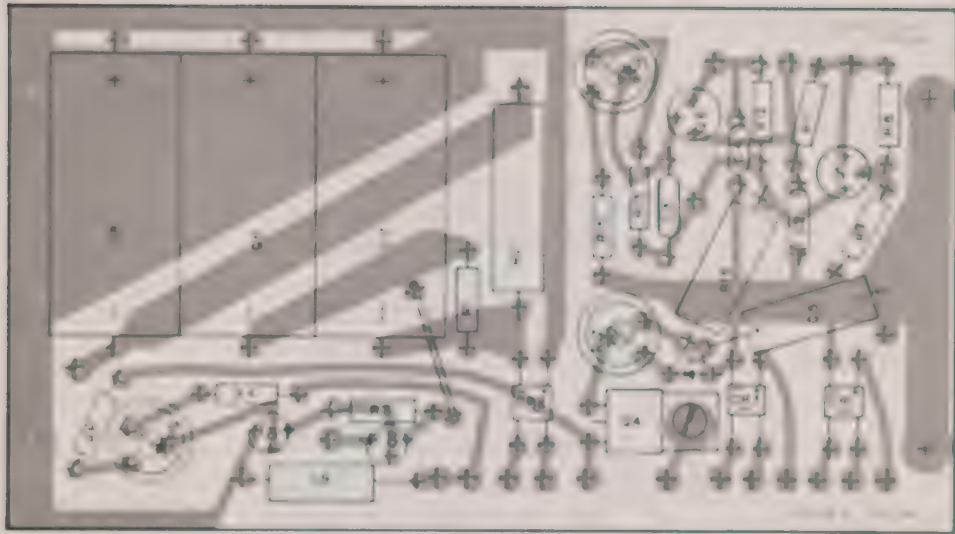


POWER SUPPLY
PCB LAYOUT

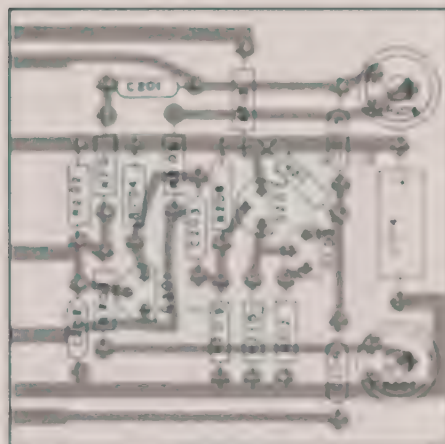


AJIO-102
 10/10/10




INCR DIST AND OUTPUT ADJUST
PR. CIR. BOARD

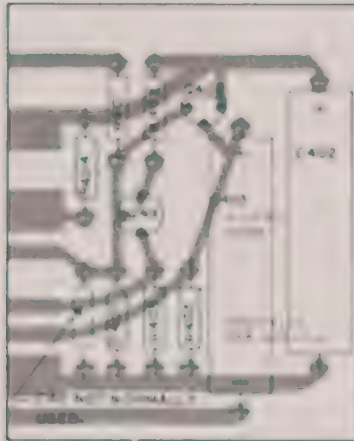

SAW TOOTH GEN
PR CIR BOARD

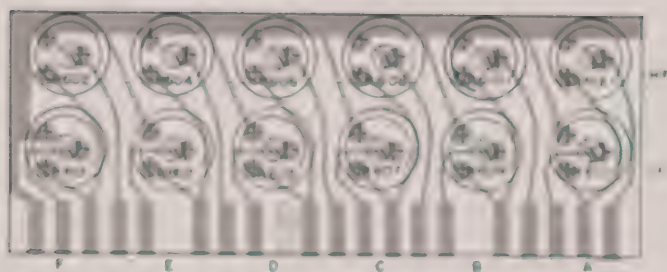

DEV. ADJ.
PR. CIR. BOARD

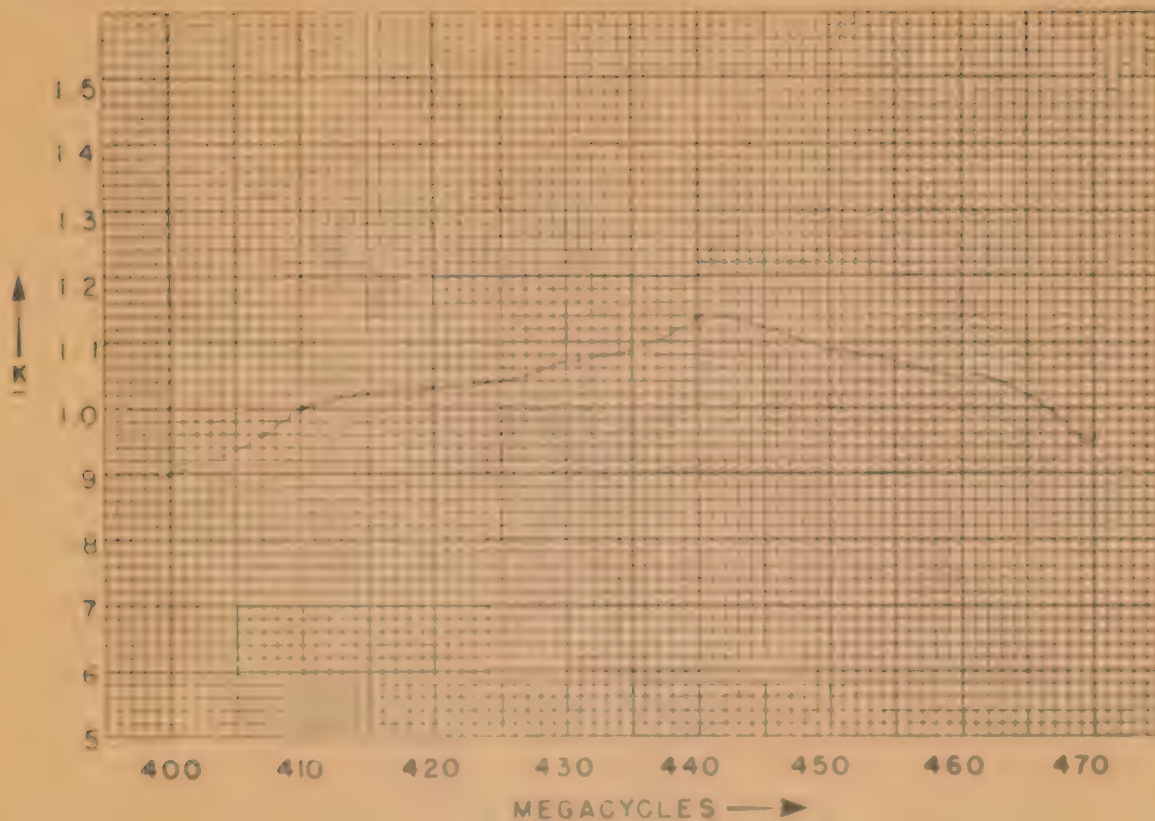

F BAND DEVIATION CORRECTION CURVE

To obtain the True Deviation make the following correction.


True Deviation in Kc = K x Meter Indication in Kc

To obtain a desired Frequency Deviation set meter KC DEVIATION
in accordance with the following:

Meter Indication in Kc = Desired Deviation in Kc

MODEL NO. 701 SERIAL NO. 1

DATE 1-2-57

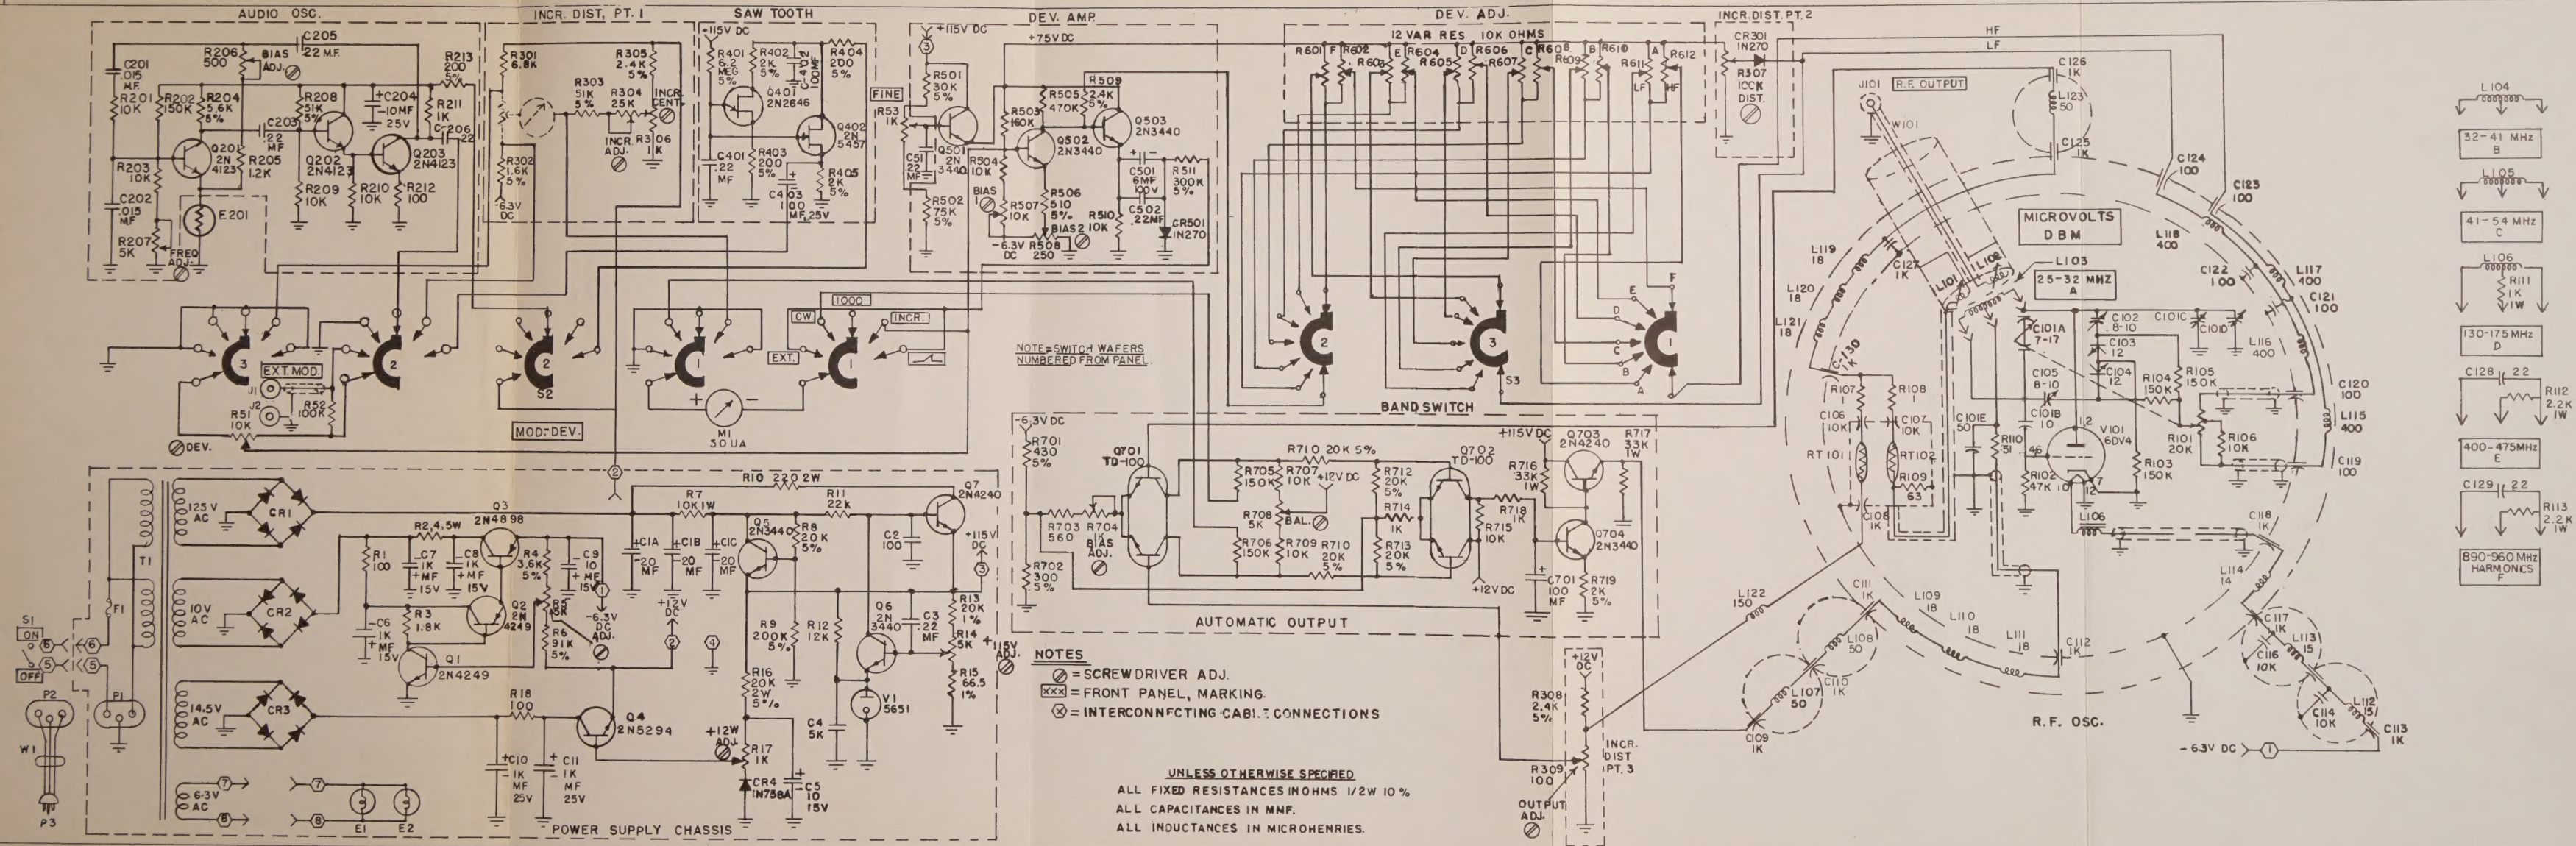

MEASUREMENTS

BOX 180, BOONTON
NEW JERSEY

